


800MHz Disaster Medical Radio System Testing

Response Compliance / April 2018 - April 2019

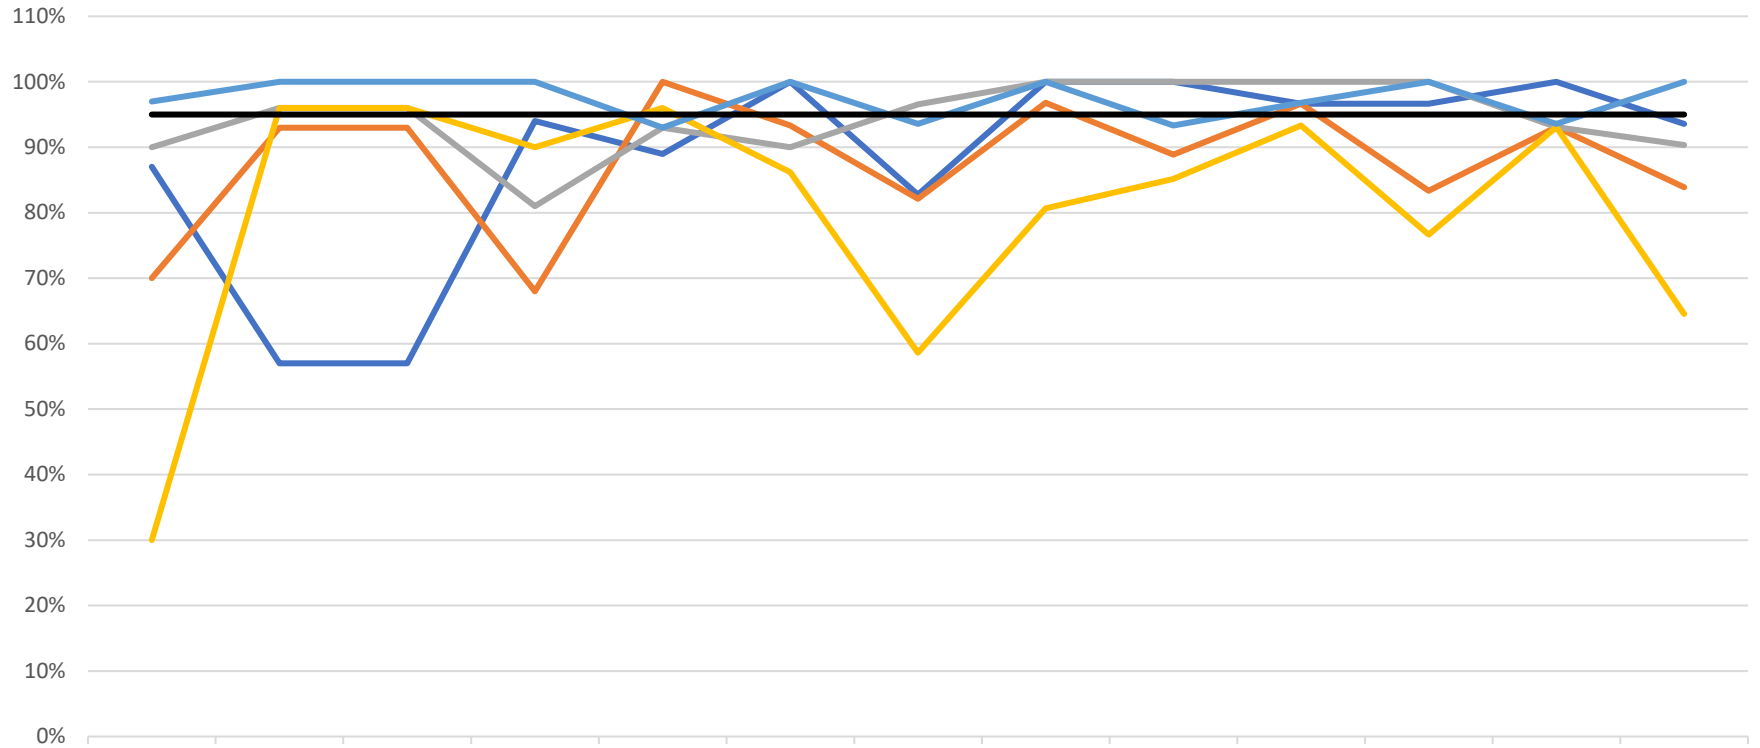


	Jan-18	Feb-18	Mar-18	Apr-18	May-18	Jun-18	Jul-18	Aug-18	Sep-18	Oct-18	Nov-18	Dec-18	Jan-19
CHOMP	87%	57%	57%	94%	89%	100%	83%	100%	100%	97%	97%	100%	94%
MMH	70%	93%	93%	68%	100%	93%	82%	97%	89%	97%	83%	93%	84%
NMC	90%	96%	96%	81%	93%	90%	97%	100%	100%	100%	100%	93%	90%
SVMH	30%	96%	96%	90%	96%	86%	59%	81%	85%	93%	77%	93%	65%
AMR	97%	100%	100%	100%	93%	100%	94%	100%	93%	97%	100%	94%	100%
STANDARD	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%

— CHOMP — MMH — NMC — SVMH — AMR — STANDARD



800MHz Disaster Medical Radio System Testing

Response Compliance / February 2018 - February 2019

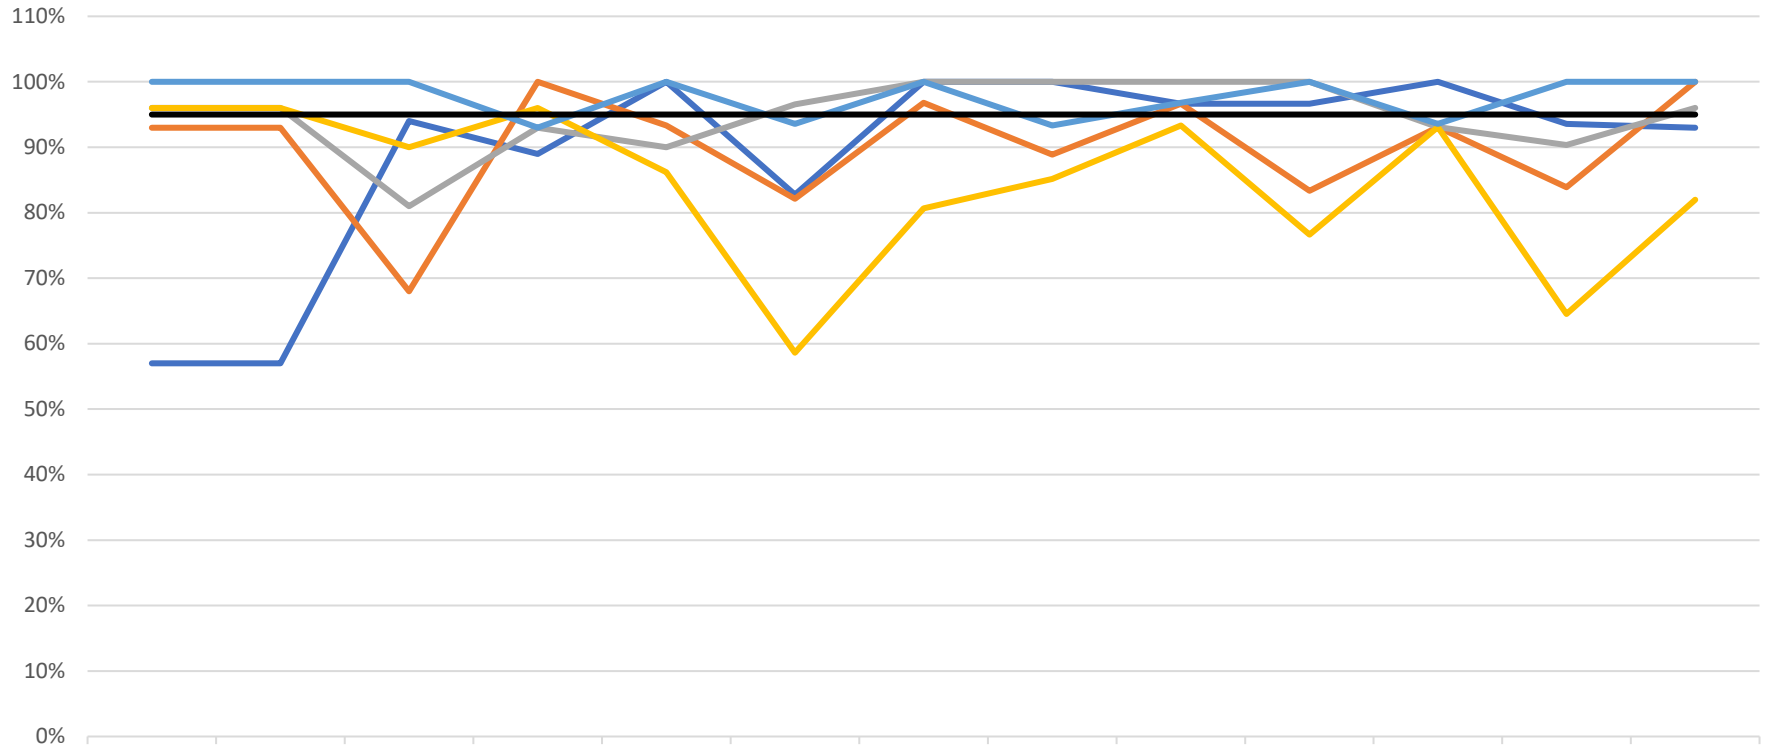


	Feb-18	Mar-18	Apr-18	May-18	Jun-18	Jul-18	Aug-18	Sep-18	Oct-18	Nov-18	Dec-18	Jan-19	Feb-19
CHOMP	57%	57%	94%	89%	100%	83%	100%	100%	97%	97%	100%	94%	93%
MMH	93%	93%	68%	100%	93%	82%	97%	89%	97%	83%	93%	84%	100%
NMC	96%	96%	81%	93%	90%	97%	100%	100%	100%	100%	93%	90%	96%
SVMH	96%	96%	90%	96%	86%	59%	81%	85%	93%	77%	93%	65%	82%
AMR	100%	100%	100%	93%	100%	94%	100%	93%	97%	100%	94%	100%	100%
STANDARD	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%

— CHOMP — MMH — NMC — SVMH — AMR — STANDARD



800MHz Disaster Medical Radio System Testing

Response Compliance / March 2018 - March 2019

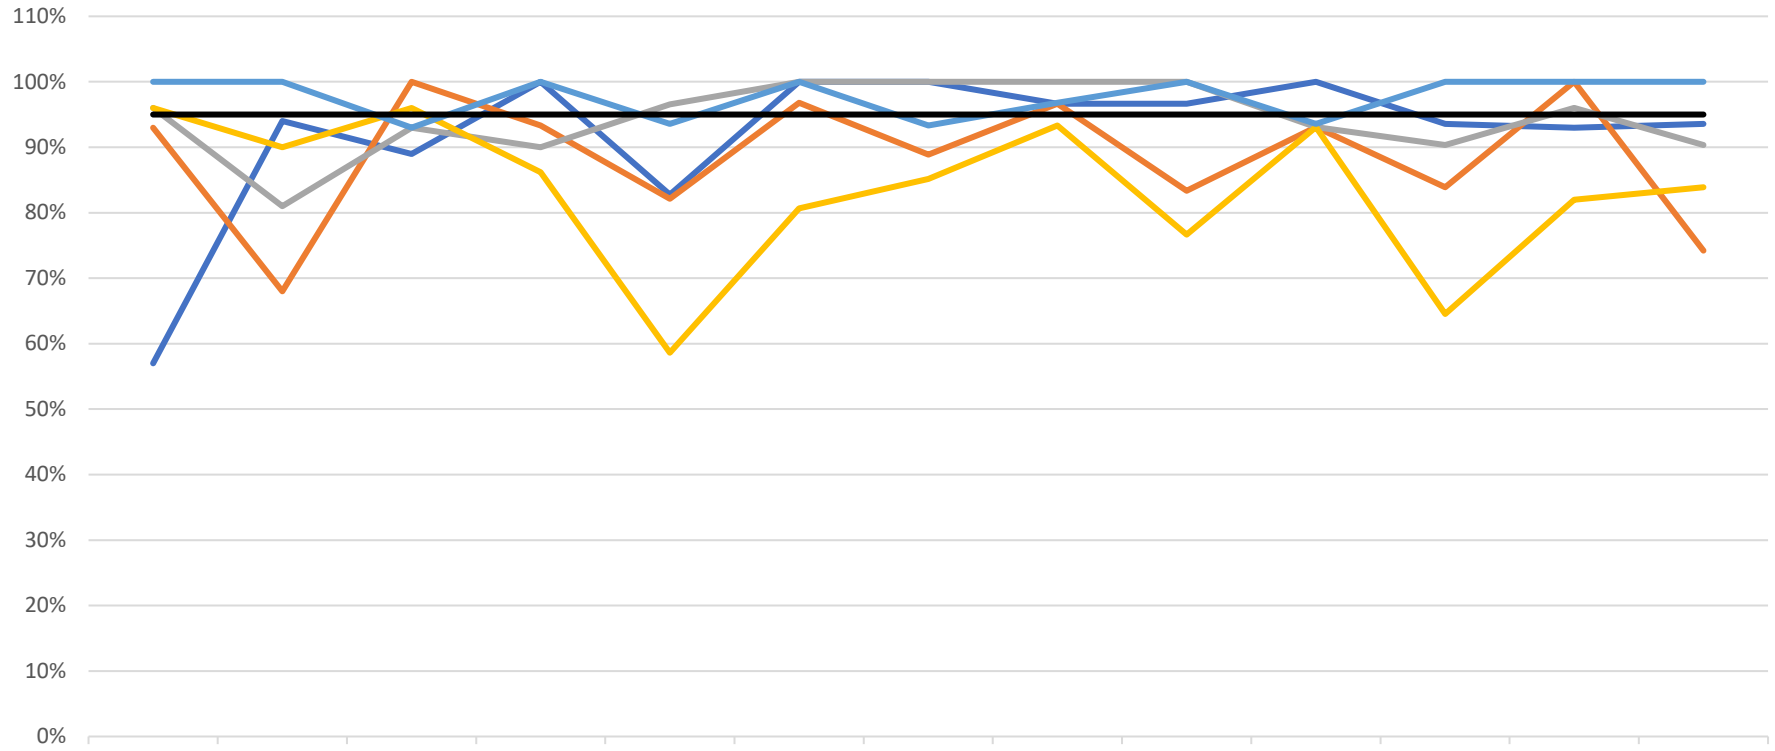


	Mar-18	Apr-18	May-18	Jun-18	Jul-18	Aug-18	Sep-18	Oct-18	Nov-18	Dec-18	Jan-19	Feb-19	Mar-19
CHOMP	57%	94%	89%	100%	83%	100%	100%	97%	97%	100%	94%	93%	94%
MMH	93%	68%	100%	93%	82%	97%	89%	97%	83%	93%	84%	100%	74%
NMC	96%	81%	93%	90%	97%	100%	100%	100%	100%	93%	90%	96%	90%
SVMH	96%	90%	96%	86%	59%	81%	85%	93%	77%	93%	65%	82%	84%
AMR	100%	100%	93%	100%	94%	100%	93%	97%	100%	94%	100%	100%	100%
STANDARD	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%

— CHOMP — MMH — NMC — SVMH — AMR — STANDARD



800MHz Disaster Medical Radio System Testing

Response Compliance / April 2018 - April 2019

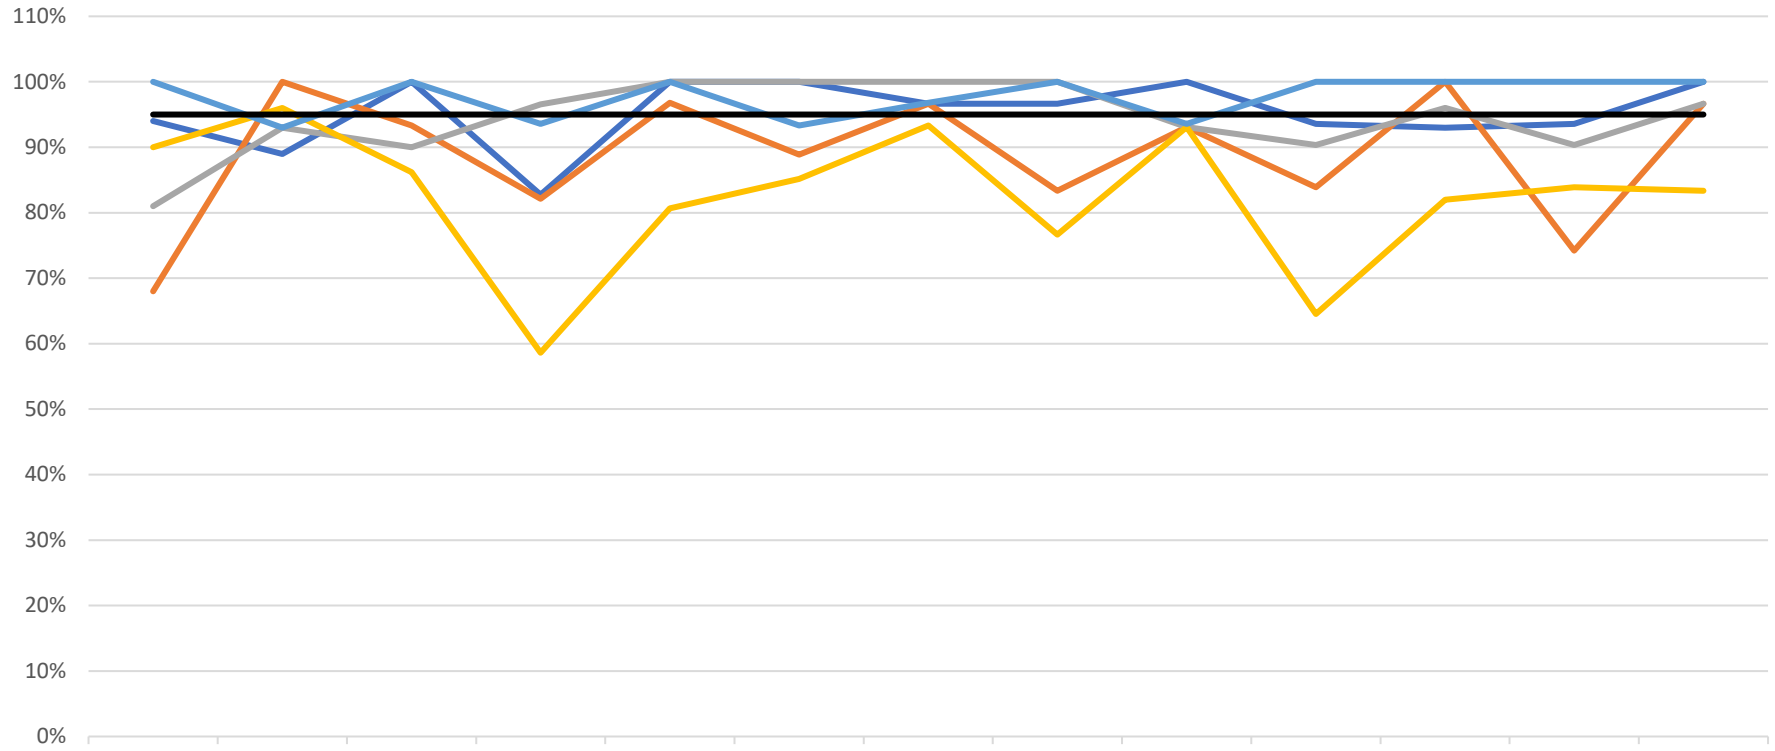


	Apr-18	May-18	Jun-18	Jul-18	Aug-18	Sep-18	Oct-18	Nov-18	Dec-18	Jan-19	Feb-19	Mar-19	Apr-19
CHOMP	94%	89%	100%	83%	100%	100%	97%	97%	100%	94%	93%	94%	100%
MMH	68%	100%	93%	82%	97%	89%	97%	83%	93%	84%	100%	74%	97%
NMC	81%	93%	90%	97%	100%	100%	100%	100%	93%	90%	96%	90%	97%
SVMH	90%	96%	86%	59%	81%	85%	93%	77%	93%	65%	82%	84%	83%
AMR	100%	93%	100%	94%	100%	93%	97%	100%	94%	100%	100%	100%	100%
STANDARD	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%

— CHOMP — MMH — NMC — SVMH — AMR — STANDARD



800MHz Disaster Medical Radio System Testing

Response Compliance / May 2018 - May 2019

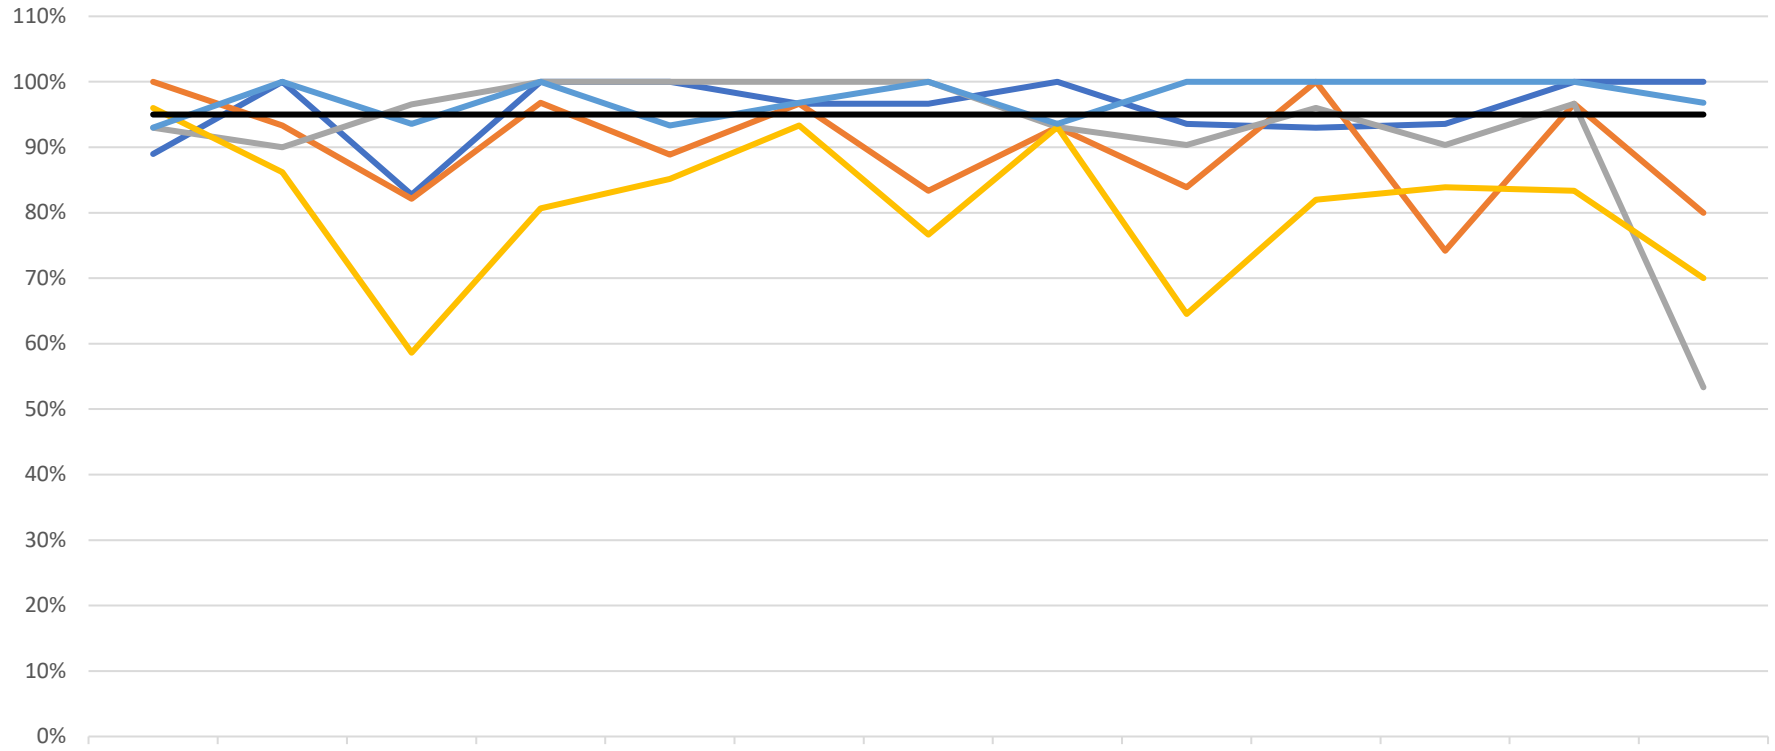


	May-18	Jun-18	Jul-18	Aug-18	Sep-18	Oct-18	Nov-18	Dec-18	Jan-19	Feb-19	Mar-19	Apr-19	May-19
CHOMP	89%	100%	83%	100%	100%	97%	97%	100%	94%	93%	94%	100%	100%
MMH	100%	93%	82%	97%	89%	97%	83%	93%	84%	100%	74%	97%	80%
NMC	93%	90%	97%	100%	100%	100%	100%	93%	90%	96%	90%	97%	53%
SVMH	96%	86%	59%	81%	85%	93%	77%	93%	65%	82%	84%	83%	70%
AMR	93%	100%	94%	100%	93%	97%	100%	94%	100%	100%	100%	100%	97%
STANDARD	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%

— CHOMP — MMH — NMC — SVMH — AMR — STANDARD



800MHz Disaster Medical Radio System Testing

Response Compliance / June 2018 - June 2019

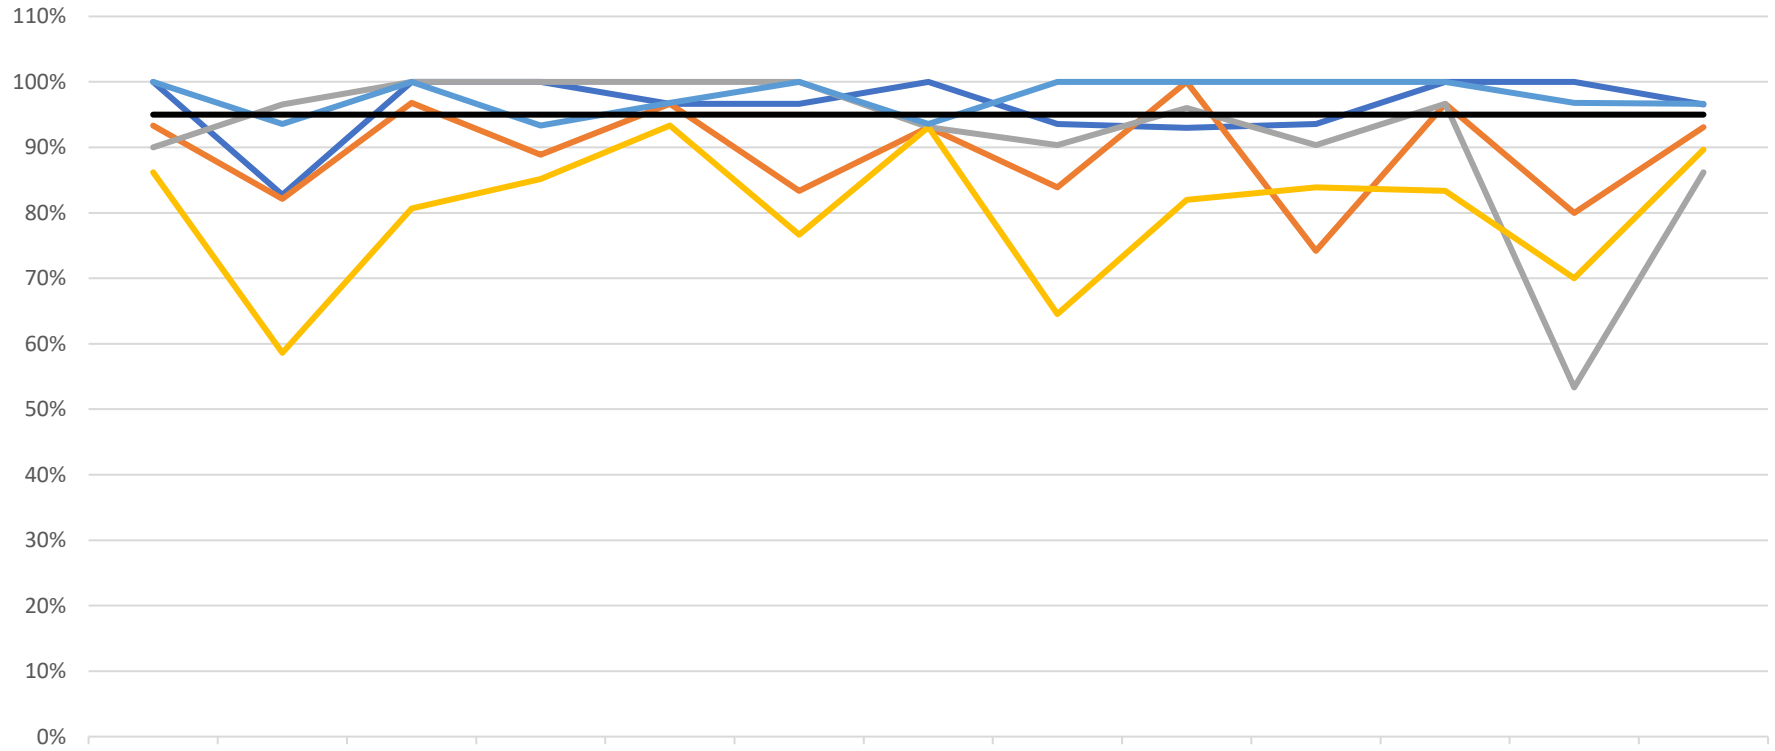


	Jun-18	Jul-18	Aug-18	Sep-18	Oct-18	Nov-18	Dec-18	Jan-19	Feb-19	Mar-19	Apr-19	May-19	Jun-19
CHOMP	100%	83%	100%	100%	97%	97%	100%	94%	93%	94%	100%	100%	97%
MMH	93%	82%	97%	89%	97%	83%	93%	84%	100%	74%	97%	80%	93%
NMC	90%	97%	100%	100%	100%	100%	93%	90%	96%	90%	97%	53%	86%
SVMH	86%	59%	81%	85%	93%	77%	93%	65%	82%	84%	83%	70%	90%
AMR	100%	94%	100%	93%	97%	100%	94%	100%	100%	100%	100%	97%	97%
STANDARD	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%

— CHOMP — MMH — NMC — SVMH — AMR — STANDARD



800MHz Disaster Medical Radio System Testing

Response Compliance / July 2018 - July 2019

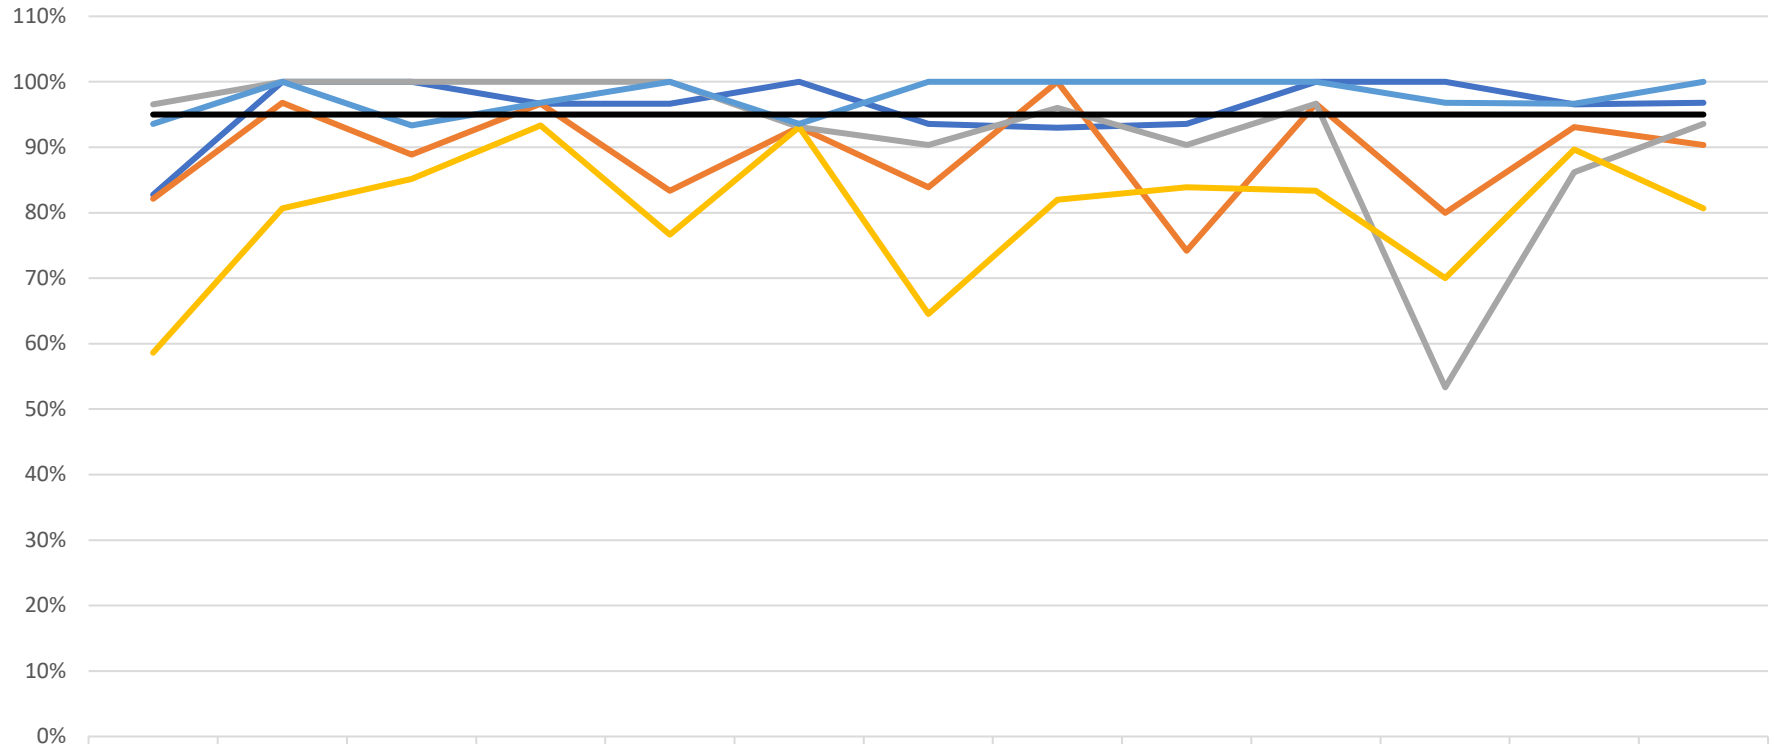


	Jul-18	Aug-18	Sep-18	Oct-18	Nov-18	Dec-18	Jan-19	Feb-19	Mar-19	Apr-19	May-19	Jun-19	Jul-19
CHOMP	83%	100%	100%	97%	97%	100%	94%	93%	94%	100%	100%	97%	97%
MMH	82%	97%	89%	97%	83%	93%	84%	100%	74%	97%	80%	93%	90%
NMC	97%	100%	100%	100%	100%	93%	90%	96%	90%	97%	53%	86%	94%
SVMH	59%	81%	85%	93%	77%	93%	65%	82%	84%	83%	70%	90%	81%
AMR	94%	100%	93%	97%	100%	94%	100%	100%	100%	100%	97%	97%	100%
STANDARD	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%

— CHOMP
 — MMH
 — NMC
 — SVMH
 — AMR
 — STANDARD



800MHz Disaster Medical Radio System Testing

Response Compliance / August 2018 - August 2019

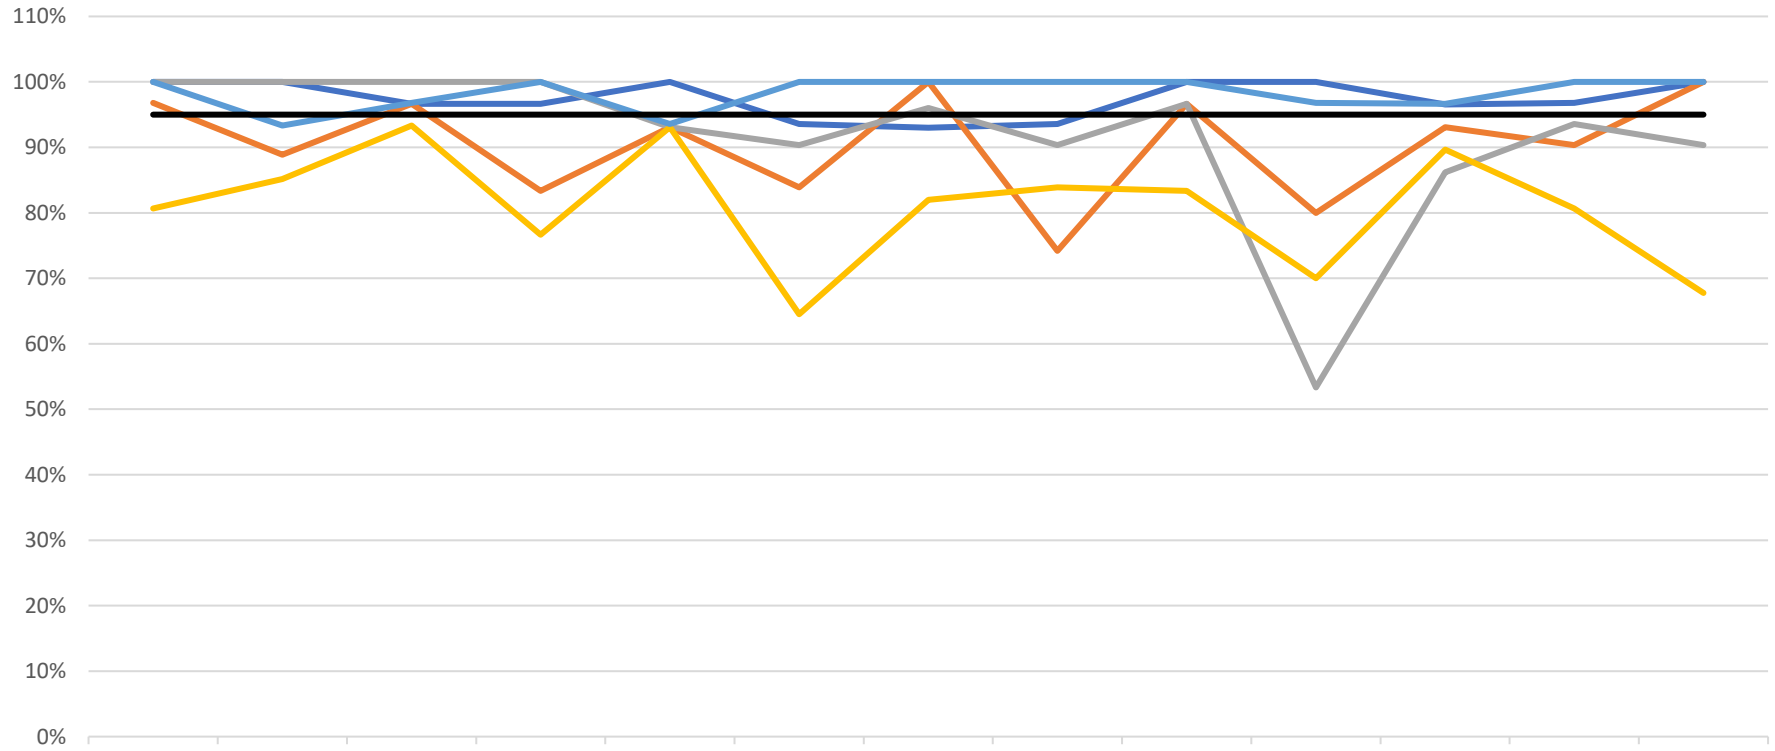


	Aug-18	Sep-18	Oct-18	Nov-18	Dec-18	Jan-19	Feb-19	Mar-19	Apr-19	May-19	Jun-19	Jul-19	Aug-19
CHOMP	100%	100%	97%	97%	100%	94%	93%	94%	100%	100%	97%	97%	100%
MMH	97%	89%	97%	83%	93%	84%	100%	74%	97%	80%	93%	90%	100%
NMC	100%	100%	100%	100%	93%	90%	96%	90%	97%	53%	86%	94%	90%
SVMH	81%	85%	93%	77%	93%	65%	82%	84%	83%	70%	90%	81%	68%
AMR	100%	93%	97%	100%	94%	100%	100%	100%	100%	97%	97%	100%	100%
STANDARD	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%

— CHOMP — MMH — NMC — SVMH — AMR — STANDARD



800MHz Disaster Medical Radio System Testing

Response Compliance / September 2018 - September 2019

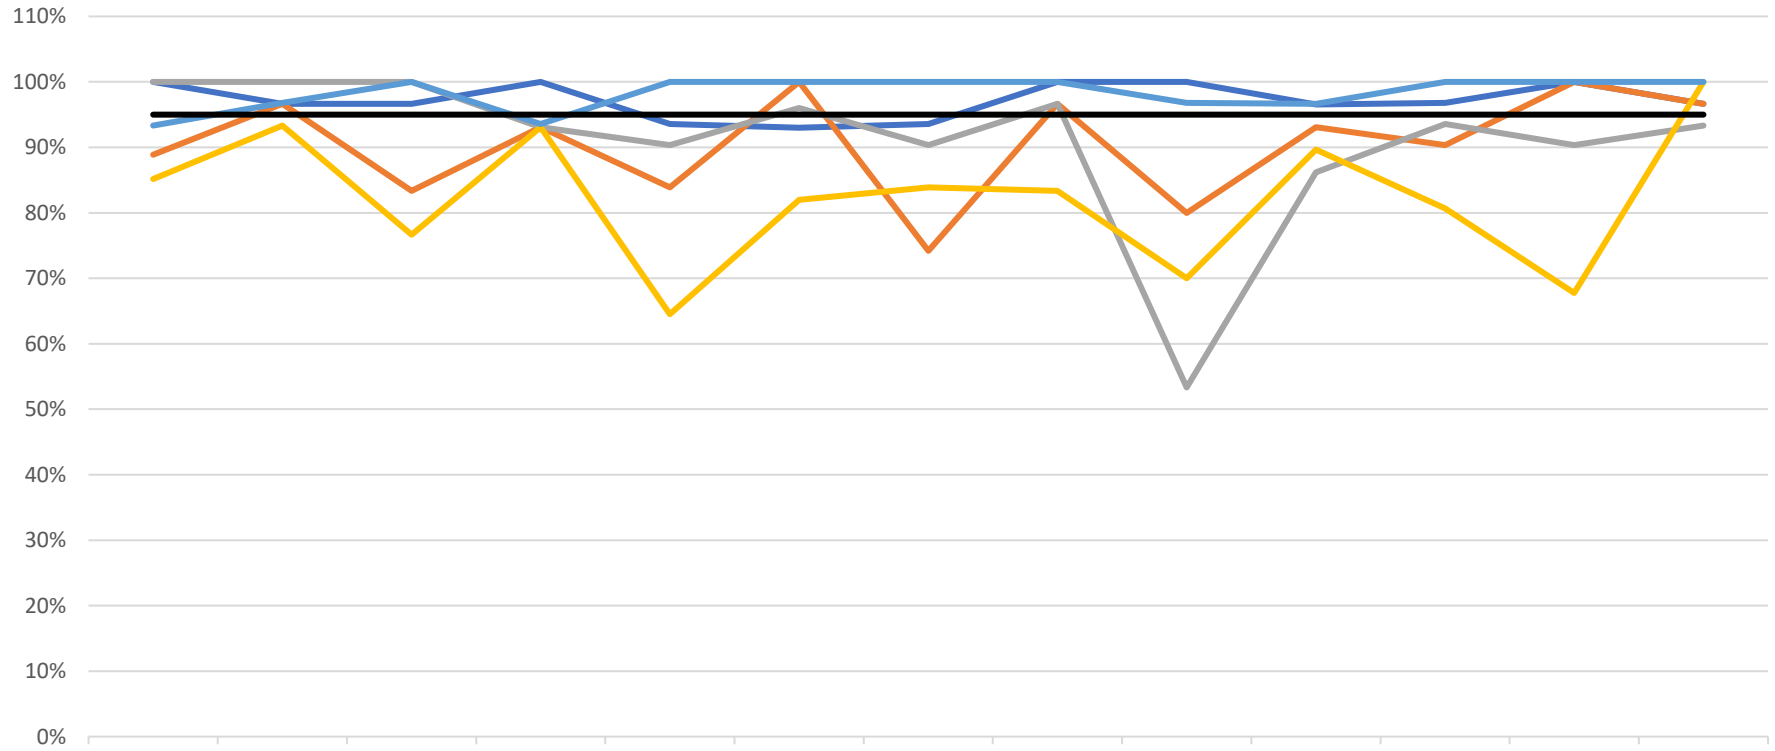


	Sep-18	Oct-18	Nov-18	Dec-18	Jan-19	Feb-19	Mar-19	Apr-19	May-19	Jun-19	Jul-19	Aug-19	Sep-19
CHOMP	100%	97%	97%	100%	94%	93%	94%	100%	100%	97%	97%	100%	97%
MMH	89%	97%	83%	93%	84%	100%	74%	97%	80%	93%	90%	100%	97%
NMC	100%	100%	100%	93%	90%	96%	90%	97%	53%	86%	94%	90%	93%
SVMH	85%	93%	77%	93%	65%	82%	84%	83%	70%	90%	81%	68%	100%
AMR	93%	97%	100%	94%	100%	100%	100%	100%	97%	97%	100%	100%	100%
STANDARD	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%

— CHOMP — MMH — NMC — SVMH — AMR — STANDARD



800MHz Disaster Medical Radio System Testing

Response Compliance / October 2018 - October 2019

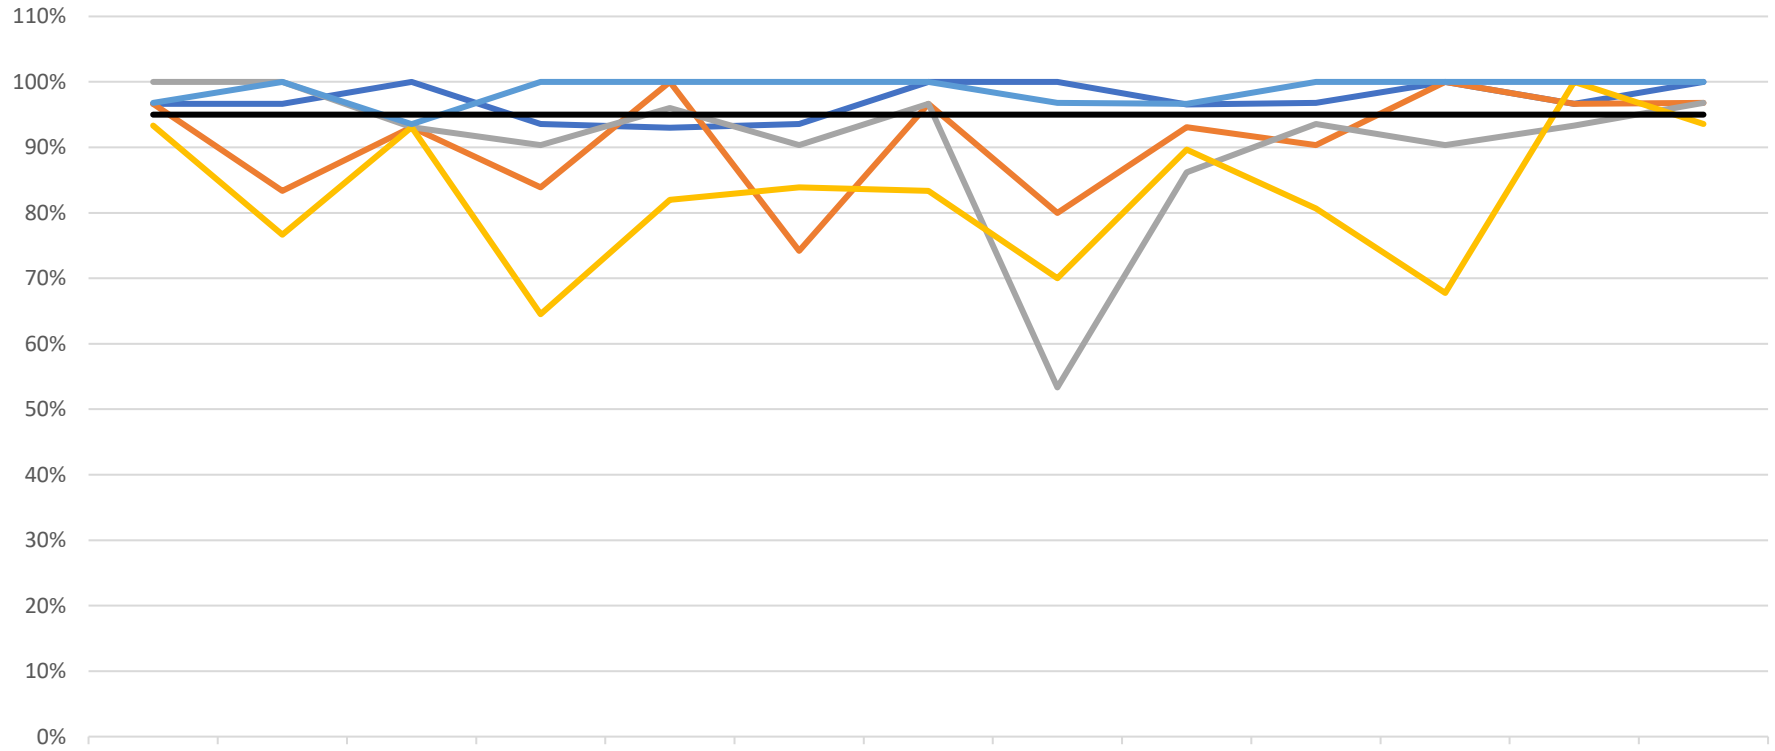


	Oct-18	Nov-18	Dec-18	Jan-19	Feb-19	Mar-19	Apr-19	May-19	Jun-19	Jul-19	Aug-19	Sep-19	Oct-19
CHOMP	97%	97%	100%	94%	93%	94%	100%	100%	97%	97%	100%	97%	100%
MMH	97%	83%	93%	84%	100%	74%	97%	80%	93%	90%	100%	97%	97%
NMC	100%	100%	93%	90%	96%	90%	97%	53%	86%	94%	90%	93%	97%
SVMH	93%	77%	93%	65%	82%	84%	83%	70%	90%	81%	68%	100%	94%
AMR	97%	100%	94%	100%	100%	100%	100%	97%	97%	100%	100%	100%	100%
STANDARD	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%

— CHOMP
 — MMH
 — NMC
 — SVMH
 — AMR
 — STANDARD



800MHz Disaster Medical Radio System Testing

Response Compliance / December 2018 - November 2019

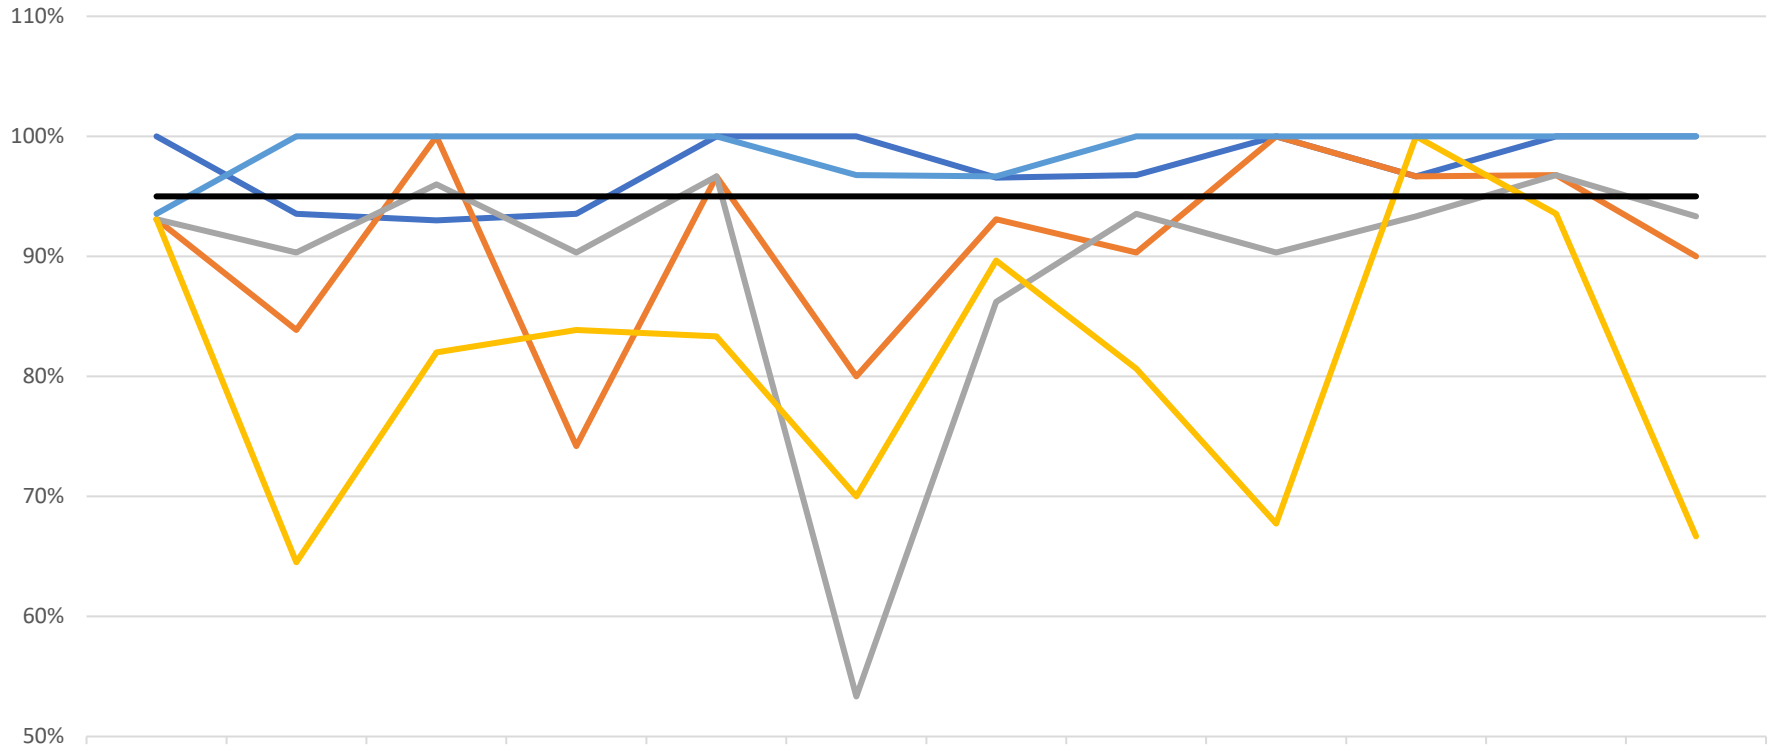


	Dec-18	Jan-19	Feb-19	Mar-19	Apr-19	May-19	Jun-19	Jul-19	Aug-19	Sep-19	Oct-19	Nov-19
CHOMP	100%	94%	93%	94%	100%	100%	97%	97%	100%	97%	100%	100%
MMH	93%	84%	100%	74%	97%	80%	93%	90%	100%	97%	97%	90%
NMC	93%	90%	96%	90%	97%	53%	86%	94%	90%	93%	97%	93%
SVMH	93%	65%	82%	84%	83%	70%	90%	81%	68%	100%	94%	67%
AMR	94%	100%	100%	100%	100%	97%	97%	100%	100%	100%	100%	100%
STANDARD	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%

— CHOMP — MMH — NMC — SVMH — AMR — STANDARD



800MHz Disaster Medical Radio System Testing

Response Compliance January 2019 - December 2019

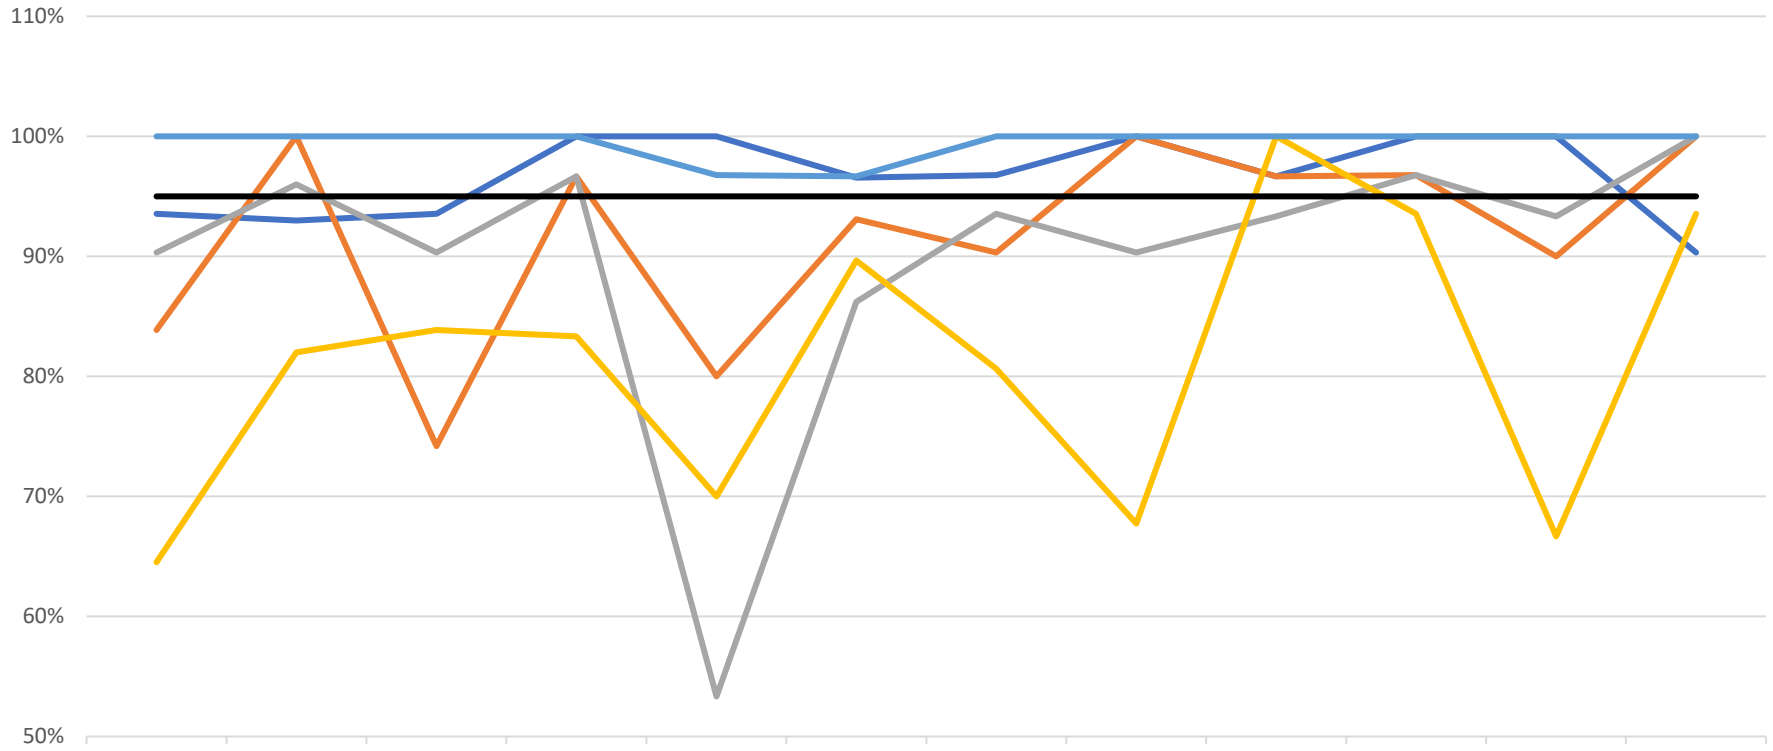

	Jan-19	Feb-19	Mar-19	Apr-19	May-19	Jun-19	Jul-19	Aug-19	Sep-19	Oct-19	Nov-19	Dec-19
CHOMP	94%	93%	94%	100%	100%	97%	97%	100%	97%	100%	100%	90%
MMH	84%	100%	74%	97%	80%	93%	90%	100%	97%	97%	90%	100%
NMC	90%	96%	90%	97%	53%	86%	94%	90%	93%	97%	93%	100%
SVMH	65%	82%	84%	83%	70%	90%	81%	68%	100%	94%	67%	94%
AMR	100%	100%	100%	100%	97%	97%	100%	100%	100%	100%	100%	100%
STANDARD	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%	95%

— CHOMP — MMH — NMC — SVMH — AMR — STANDARD

